

## Continuous Glucose Monitoring (CGM) Device Summary


Device	Works with	Provided through NDSS subsidy	Product lifespan	Other features
Dexcom G6	Compatible iOS (Apple) or Android smartphone or smart device OR Tandem t:slim X2 Insulin Pump OR mylife YpsoPump	Dexcom G6 Sensor  Dexcom G6 Transmitter <sup>4</sup>	Sensor – 10 days  Transmitter – 3 months	No calibration required.
Medtronic Guardian Connect (3) <sup>4</sup>	Compatible iOS or Android smartphone or smart device	Guardian Sensor (3)  Guardian Connect (3) Transmitter <sup>4</sup>	Sensors – 7 days  Transmitter - 12 months	
Medtronic Guardian Link (3)	Medtronic MiniMed 670G or MiniMed 640G insulin pumps	Guardian Sensor (3)  Medtronic Guardian Link (3) Transmitter	Sensors – 7 days  Transmitter - 12 months	
Medtronic Bluetooth Guardian Link (3)	Medtronic MiniMed 770G or MiniMed 780G insulin pump	Guardian Sensor (3)  Medtronic Bluetooth Guardian Link (3) Transmitter	Sensors – 7 days  Transmitter - 12 months	



## Compatibility Flowchart



How do you want to connect to your CGM device?

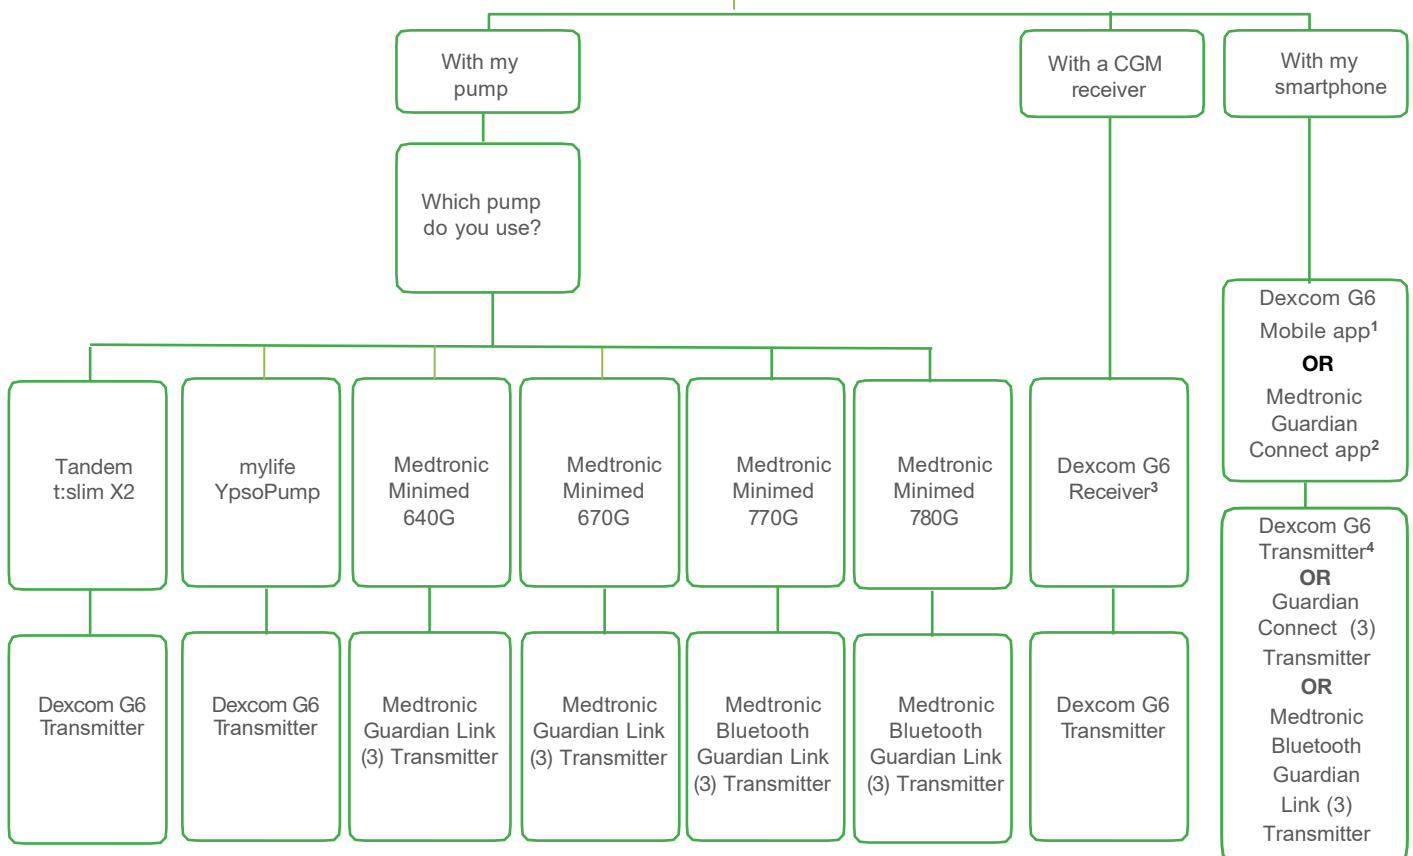

1. For information about compatible Apple iOS and Android devices for use with the Dexcom G6 visit: [dexcom.com/ous-compatibility-page](https://dexcom.com/ous-compatibility-page).
2. For information about compatible Apple iOS and Android devices for use with the Guardian Connect visit: [medtronic-diabetes.com.au/guardian-connect](https://medtronic-diabetes.com.au/guardian-connect).
3. The Dexcom G6 receiver is an alternative to using a compatible iOS or Android device and does not require cellular data or Wi-Fi connectivity. It is not subsidised through the CGM Initiative and can be purchased separately through AMSL. For more details, visit [amsldiabetes.com.au/shop](https://amsldiabetes.com.au/shop).
4. The Medtronic Guardian Connect and Dexcom G6 transmitters must be synced to a compatible Apple iOS or Android device with Bluetooth connectivity. After syncing the apps will function without cellular data or Wi-Fi connectivity. However, for sharing services to work you will need access to regular cellular data or Wi-Fi connectivity.

## CGM Device Information and Australian Register of Therapeutic Goods (ARTG) Certificates

CGM Product Name	ARTG link	Product Information Link
<b>AMSL</b>		
Dexcom G6	<a href="#">ARTG Certificate 330535</a>	<a href="#">Dexcom G6 user guide</a>
<b>Medtronic</b>		
Medtronic Enlite Sensor	<a href="#">ARTG Certificate 313740</a>	<a href="#">Medtronic Enlite Sensor user guide</a>
Medtronic Guardian Sensor (3)	<a href="#">ARTG Certificate 313741</a>	<a href="#">Medtronic Guardian Sensor (3) user guide</a>
Medtronic Guardian Link (3) Transmitter Kit	<a href="#">ARTG Certificate 138452</a>	<a href="#">Medtronic Guardian Link (3) Transmitter user guide</a>
Medtronic Guardian Link (3) Transmitter (Stand-alone)	<a href="#">ARTG Certificate 118347</a>	
Medtronic Guardian Connect(3) Transmitter Kit [for Guardian Sensor (3)]	<a href="#">ARTG Certificate 138452</a>	<a href="#">Medtronic Guardian Connect (3) Transmitter user guide</a>
Medtronic Guardian Link (3) Transmitter (Stand-alone) [for Guardian Sensor (3)]	<a href="#">ARTG Certificate 118347</a>	
Medtronic Bluetooth Guardian Link (3) Transmitter Kit	<a href="#">ARTG Certificate 118347</a>	<a href="#">Medtronic Bluetooth Guardian Link (3) Transmitter user guide</a>
Medtronic Bluetooth Guardian Link (3) Transmitter (stand-alone)	<a href="#">ARTG Certificate 118347</a>	

## Flash Glucose Monitoring (Flash GM) Device Summary

Device	Works with	Provided through NDSS subsidy	Product lifespan	Other features
FreeStyle Libre 2	FreeStyle Libre 2 reader or compatible smartphone or device <sup>1,2</sup> .	FreeStyle Libre 2 sensor	Sensor – 14 days	FreeStyle Libre 2 has optional real-time alarms for high or low glucose levels and signal loss.

1. For information about compatible smartphone or devices for use with FreeStyle Libre visit: [freestylelibre.com.au/glucose-monitoring-system/support](https://freestylelibre.com.au/glucose-monitoring-system/support).
2. Glucose data is displayed after every scan by the reader or using the FreeStyle LibreLink app on your smartphone or device. For more information see the FreeStyle product information link in the table below.

## Flash GM Device Information and Australian Register of Therapeutic Goods (ARTG) Certificates

Product name	ARTG link	Product information link
<b>Abbott</b>		
FreeStyle Libre 2 system	<a href="#">ARTG certificate 358292</a>	<a href="#">FreeStyle Libre 2 Quick Start Guide</a>